

# INTERNATIONAL STANDARD

# IEC 60601-2-2

Third edition  
1998-09

---

---

## Medical electrical equipment –

### Part 2-2: Particular requirements for the safety of high frequency surgical equipment

*Appareils électromédicaux –*

*Partie 2-2:  
Règles particulières de sécurité pour appareils  
d'électrochirurgie à courant haute fréquence*

© IEC 1998 — Copyright - all rights reserved

No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Electrotechnical Commission  
Telefax: +41 22 919 0300

3, rue de Varembé Geneva, Switzerland  
e-mail: [inmail@iec.ch](mailto:inmail@iec.ch) IEC web site <http://www.iec.ch>



Commission Electrotechnique Internationale  
International Electrotechnical Commission  
Международная Электротехническая Комиссия

PRICE CODE

X

For price, see current catalogue

## CONTENTS

	Page
FOREWORD .....	4
INTRODUCTION .....	6
Clause	
<b>SECTION ONE – GENERAL</b>	
1 Scope and object .....	7
2 Terminology and definitions .....	8
3 General requirements .....	9
4 General requirements for tests .....	10
5 Classification .....	10
6 Identification, marking and documents .....	10
7 Power input .....	13
<b>SECTION TWO – ENVIRONMENTAL CONDITIONS</b>	
<b>SECTION THREE – PROTECTION AGAINST ELECTRICAL SHOCK HAZARDS</b>	
14 Requirements related to classification .....	14
17 Separation .....	14
18 Protective earthing, functional earthing and potential equalization .....	14
19 Continuous LEAKAGE CURRENTS and PATIENT AUXILIARY CURRENTS .....	14
20 Dielectric strength .....	17
<b>SECTION FOUR – PROTECTION AGAINST MECHANICAL HAZARDS</b>	
<b>SECTION FIVE – PROTECTION AGAINST HAZARDS FROM UNWANTED OR EXCESSIVE RADIATION</b>	
36 Electromagnetic compatibility .....	18
<b>SECTION SIX – PROTECTION AGAINST HAZARDS OF IGNITION OF FLAMMABLE ANAESTHETIC MIXTURES</b>	
39 Common requirements for CATEGORY AP and CATEGORY APG EQUIPMENT .....	19

SECTION SEVEN – PROTECTION AGAINST EXCESSIVE TEMPERATURES  
AND OTHER SAFETY HAZARDS

42 Excessive temperatures .....	19
44 Overflow, spillage, leakage, humidity, ingress of liquids, cleaning, sterilization, disinfection and compatibility .....	19
46 Human errors .....	20

SECTION EIGHT – ACCURACY OF OPERATING DATA AND PROTECTION  
AGAINST HAZARDOUS OUTPUT

50 Accuracy of operating data .....	21
51 Protection against hazardous output .....	22

SECTION NINE – ABNORMAL OPERATION AND FAULT CONDITIONS;  
ENVIRONMENTAL TESTS


52 Abnormal operation and fault conditions .....	24
--	----

SECTION TEN – CONSTRUCTIONAL REQUIREMENTS

56 Components and general assembly .....	24
59 Construction and layout .....	26

Figures 101 to 109 .....	29–33
--------------------------	-------

Appendix L References – Publications mentioned in this standard .....	34
Annex AA (informative) Guidance and rationale for particular clauses and subclauses....	35

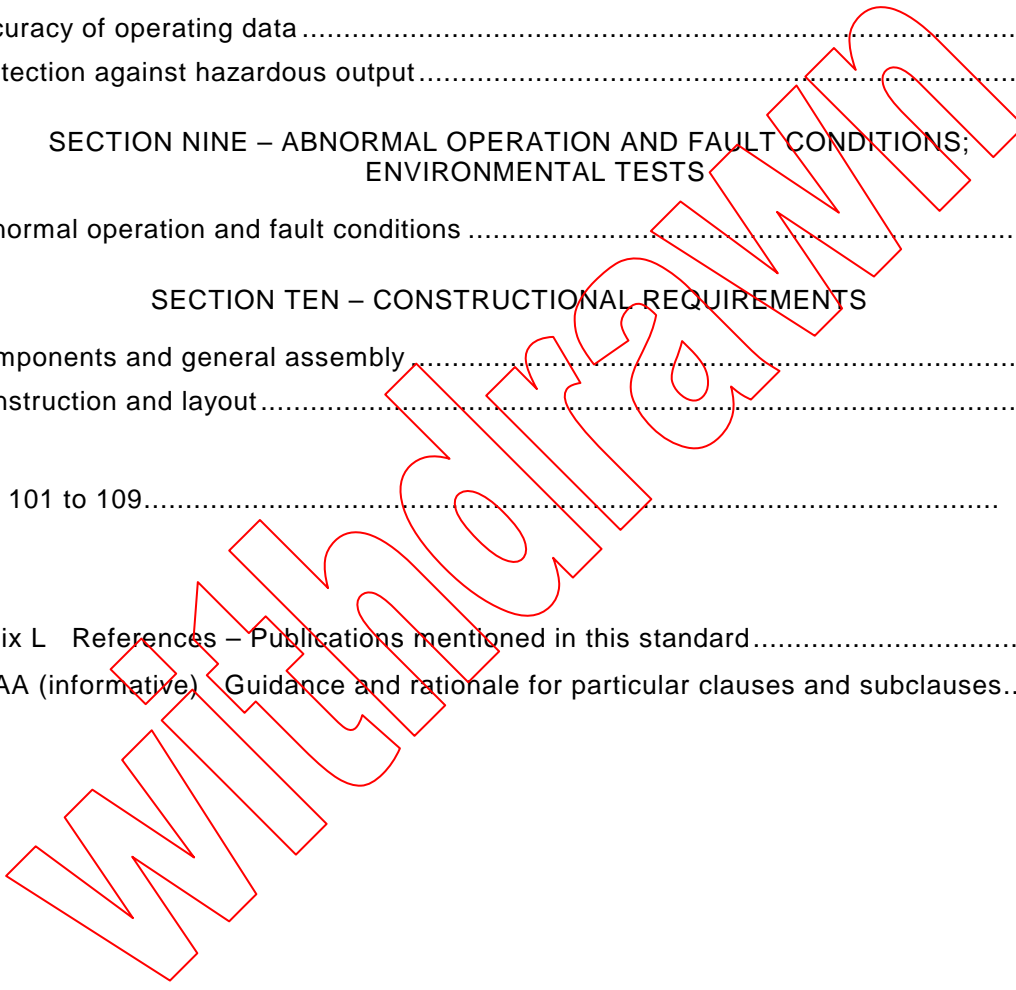

# INTERNATIONAL ELECTROTECHNICAL COMMISSION

## MEDICAL ELECTRICAL EQUIPMENT –

### Part 2-2: Particular requirements for the safety of high frequency surgical equipment

#### FOREWORD

- 1) The IEC (International Electrotechnical Commission) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of the IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, the IEC publishes International Standards. Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. The IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of the IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested National Committees.
- 3) The documents produced have the form of recommendations for international use and are published in the form of standards, technical reports or guides and they are accepted by the National Committees in that sense.
- 4) In order to promote international unification, IEC National Committees undertake to apply IEC International Standards transparently to the maximum extent possible in their national and regional standards. Any divergence between the IEC Standard and the corresponding national or regional standard shall be clearly indicated in the latter.
- 5) The IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with one of its standards.
- 6) Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. The IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 60601-2-2 has been prepared by subcommittee 62D: Electromedical equipment, of IEC technical committee 62: Electrical equipment in medical practice

This third edition of IEC 60601-2-2 cancels and replaces the second edition published in 1991, and constitutes a technical revision.

The text of this Particular Standard is based on the following documents:

FDIS	Report on voting
62D/291/FDIS	62D/297/RVD

Full information on the voting for the approval of this Particular Standard can be found in the report on voting indicated in the above table.

Annex AA is for information only.

In this Particular Standard the following print types are used:

- requirements, compliance with which can be tested, and definitions: in roman type;
- notes, explanations, advice, introductions, general statements, exceptions and references: in smaller type;
- *test specifications: in italic type;*
- TERMS DEFINED IN CLAUSE 2 OF THE GENERAL STANDARD OR THIS PARTICULAR STANDARD:  
SMALL CAPITALS.

Withdrawn

## INTRODUCTION

The revisions for this third edition of the Particular Standard refer mainly to the following:

- Split NEUTRAL ELECTRODES are dealt with in more detail.
- Limitation of incorrect output power in SINGLE FAULT CONDITION.
- The requirements for AP EQUIPMENT are revised.
- White indicator lamps on coloured backgrounds for CUTTING and COAGULATION mode are no longer allowed.
- Limitation of monitoring current to 100  $\mu$ A for HF SURGICAL EQUIPMENT with BF or CF APPLIED PARTS.
- Revised requirements for CREEPAGE DISTANCE and AIR CLEARANCE of APPLIED PARTS.
- Simultaneous activation of more than one PATIENT CIRCUIT is dealt with in more detail and a compliance test method is now defined.

Withdrawal

## MEDICAL ELECTRICAL EQUIPMENT –

### Part 2-2: Particular requirements for the safety of high frequency surgical equipment

#### SECTION ONE – GENERAL

The clauses and subclauses of this section of the General Standard apply except as follows:

#### 1 Scope and object

This clause of the General Standard applies except as follows:

##### \*1.1 Scope

*Addition:*

This Particular Standard specifies requirements for the safety of HIGH FREQUENCY SURGICAL EQUIPMENT used in medical practice, as defined in 2.1.101 and hereinafter referred to as HF SURGICAL EQUIPMENT.

HF SURGICAL EQUIPMENT having a RATED OUTPUT POWER not exceeding 50 W (for example for micro-coagulation, or for use in dentistry or ophthalmology) is exempt from certain of the requirements of this Particular Standard. These exemptions are indicated in the relevant requirements.

##### 1.2 Object

*Replacement:*

The object of this Particular Standard is to establish particular requirements for the safety of HF SURGICAL EQUIPMENT.

##### 1.3 Particular Standards

*Addition:*

This Particular Standard amends and supplements a set of IEC publications consisting of

IEC 60601-1:1988, *Medical electrical equipment – Part 1: General requirements for safety*  
Amendment 1 (1991)  
Amendment 2 (1995)

IEC 60601-1-1:1992, *Medical electrical equipment – Part 1: General requirements for safety – 1: Collateral Standard: Safety requirements for medical electrical systems*

IEC 60601-1-2:1993, *Medical electrical equipment – Part 1: General requirements for safety – 2: Collateral Standard: Electromagnetic compatibility – Requirements and tests*

IEC 60601-1-4:1996, *Medical electrical equipment – Part 1: General requirements for safety – 4: Collateral Standard: Programmable electrical medical systems*