



IEC 60601-2-46

Edition 3.0 2016-08  
REDLINE VERSION

# INTERNATIONAL STANDARD

Medical electrical equipment –  
Part 2-46: Particular requirements for the basic safety and essential  
performance of operating tables



INTERNATIONAL  
ELECTROTECHNICAL  
COMMISSION

ICS 11.140

ISBN 978-2-8322-3581-2

**Warning! Make sure that you obtained this publication from an authorized distributor.**

## CONTENTS

FOREWORD .....	3
INTRODUCTION .....	6
201.1 Scope, object and related standards .....	7
201.2 Normative references .....	9
201.3 Terms and definitions .....	9
201.4 General requirements .....	10
201.5 General requirements for testing <del>ME EQUIPMENT</del> OPERATING TABLES .....	10
201.6 Classification of <del>ME EQUIPMENT</del> OPERATING TABLES and ME SYSTEMS .....	10
201.7 <del>ME EQUIPMENT</del> OPERATING TABLES identification, marking and documents .....	11
201.8 Protection against electrical HAZARDS from <del>ME EQUIPMENT</del> OPERATING TABLES .....	11
201.9 Protection against MECHANICAL HAZARDS of <del>ME EQUIPMENT</del> OPERATING TABLES and ME SYSTEMS .....	11
201.10 Protection against unwanted and excessive radiation HAZARDS .....	14
201.11 Protection against excessive temperatures and other HAZARDS .....	14
201.12 Accuracy of controls and instruments and protection against hazardous outputs .....	15
201.13 HAZARDOUS SITUATIONS and fault conditions for OPERATING TABLES .....	15
201.14 PROGRAMMABLE ELECTRICAL MEDICAL SYSTEMS (PEMS) .....	15
201.15 Construction of <del>ME EQUIPMENT</del> OPERATING TABLES .....	15
201.16 ME SYSTEMS .....	15
201.17 Electromagnetic compatibility of <del>ME EQUIPMENT</del> OPERATING TABLES and ME SYSTEMS .....	16
202 Electromagnetic <del>compatibility</del> disturbances – Requirements and tests .....	16
203 Radiation protection in diagnostic X-ray equipment .....	20
Annexes .....	21
Annex G (normative) Protection against HAZARDS of ignition of flammable anaesthetic mixtures .....	22
Annex AA (informative) Particular guidance and rationale .....	23
Bibliography .....	25
Index of defined terms used in this particular standard .....	26
Figure 202.101 – ENCLOSURE ad hoc test .....	18
Figure 202.102 – POWER SUPPLY CORD ad hoc test .....	19
Figure 202.103 – ACCESSORY cable ad hoc test .....	19
Figure AA.1 – Recommended distribution of mass in excess of 135 kg and examples of application .....	23
Table 201.101 – Determination of TENSILE SAFETY FACTOR .....	13
Table AA.1 – Recommended distribution of mass in excess of 135 kg and examples of application .....	24

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

### MEDICAL ELECTRICAL EQUIPMENT –

#### Part 2-46: Particular requirements for the basic safety and essential performance of operating tables

#### FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

This redline version of the official IEC Standard allows the user to identify the changes made to the previous edition. A vertical bar appears in the margin wherever a change has been made. Additions are in green text, deletions are in strikethrough red text.

International standard IEC 60601-2-46 has been prepared by IEC subcommittee 62D Electromedical equipment, of IEC technical committee 62: Electrical equipment in medical practice.

This third edition cancels and replaces the second edition published in 2010 and constitutes a technical revision. This edition of IEC 60601-2-46 was revised to align structurally with the 2005 edition of IEC 60601-1 and with IEC 60601-1:2005/AMD1:2012.

The text of this standard is based on the following documents:

FDIS	Report on voting
62D/1365/FDIS	62D/1371/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

In this standard, the following print types are used:

- Requirements and definitions: roman type
- *Test specifications: italic type.*
- Informative material appearing outside of tables, such as notes, examples and references: in smaller type. Normative text of tables is also in a smaller type.
- TERMS DEFINED IN CLAUSE 3 OF THE GENERAL STANDARD, IN THIS PARTICULAR STANDARD OR AS NOTED: SMALL CAPITALS.

In referring to the structure of this standard, the term

- “clause” means one of the numbered divisions within the table of contents, inclusive of all subdivisions (e.g. Clause 7 includes subclauses 7.1, 7.2, etc.);
- “subclause” means a numbered subdivision of a clause (e.g. 7.1, 7.2 and 7.2.1 are all subclauses of Clause 7).

References to clauses within this standard are preceded by the term “Clause” followed by the clause number. References to subclauses within this particular standard are by number only.

In this standard, the conjunctive “or” is used as an “inclusive or” so a statement is true if any combination of the conditions is true.

The verbal forms used in this standard conform to usage described in Annex H of the ISO/IEC Directives, Part 2. For the purposes of this standard, the auxiliary verb:

- “shall” means that compliance with a requirement or a test is mandatory for compliance with this standard;
- “should” means that compliance with a requirement or a test is recommended but is not mandatory for compliance with this standard;
- “may” is used to describe a permissible way to achieve compliance with a requirement or test.


An asterisk (\*) as the first character of a title or at the beginning of a paragraph or table title indicates that there is guidance or rationale related to that item in Annex AA.

A list of all parts of the IEC 60601 series, published under the general title *Medical electrical equipment*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC website under "http://webstore.iec.ch" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

**IMPORTANT – The “colour inside” logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this publication using a colour printer.**

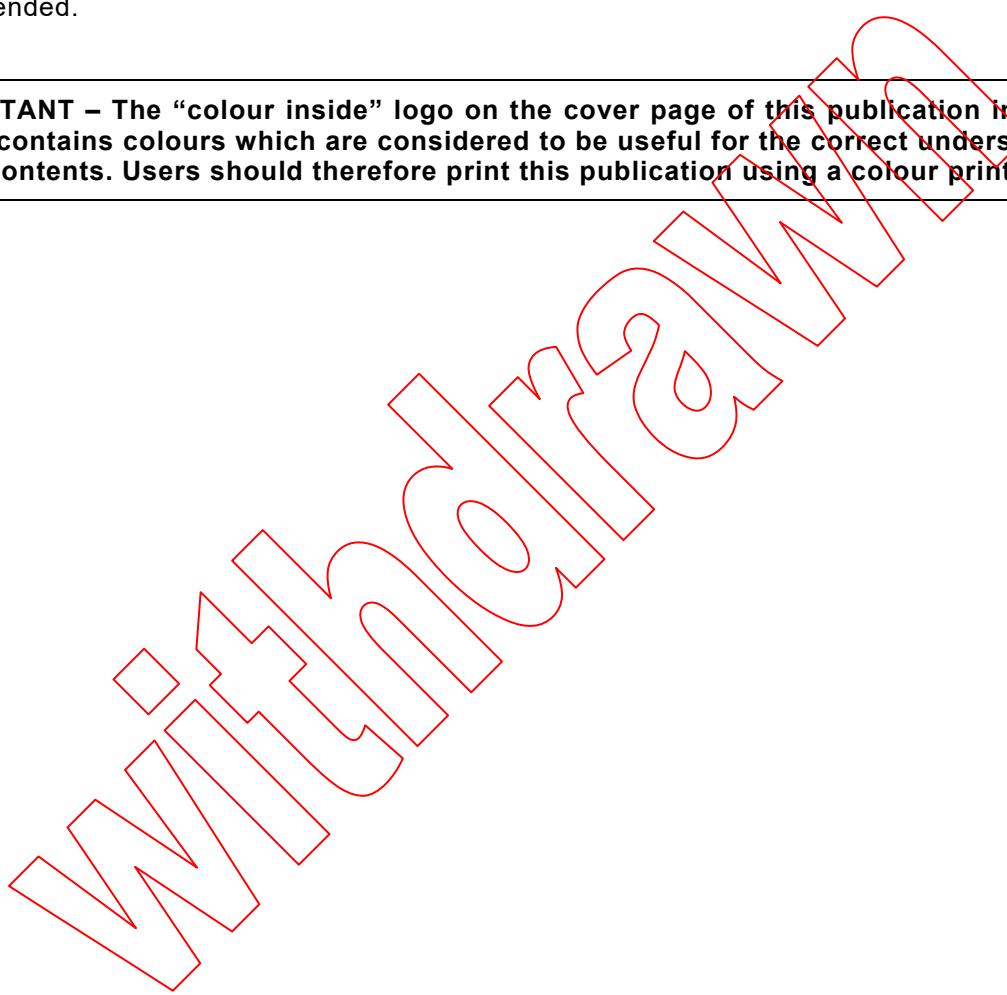

## INTRODUCTION

This particular standard concerns the BASIC SAFETY and ESSENTIAL PERFORMANCE of OPERATING TABLES. It amends and supplements IEC 60601-1 (third edition, 2005): ~~Medical electrical equipment Part 1: General requirements for basic safety and essential performance~~ and its Amendment 1 (IEC 60601-1:2005/AMD1:2012), hereinafter referred to as the general standard.

The aim of this third edition is to bring this particular standard up to date with reference to the third edition of the general standard through reformatting and technical changes.

The requirements of this particular standard take priority over those of the general standard.

A “General guidance and rationale” for the more important requirements of this particular standard is included in Annex AA. It is considered that knowledge of the reasons for these requirements will not only facilitate the proper application of the standard but will, in due course, expedite any revision necessitated by changes in clinical practice or as a result of developments in technology. However, Annex AA does not form part of the requirements of this Standard.

~~With which~~

## MEDICAL ELECTRICAL EQUIPMENT –

### Part 2-46: Particular requirements for the basic safety and essential performance of operating tables

#### 201.1 Scope, object and related standards

Clause 1 of the general standard<sup>1)</sup> applies, except as follows:

##### 201.1.1 Scope

*Replacement:*

This particular standard specifies safety requirements for OPERATING TABLES, whether or not having electrical parts, including TRANSPORTERS, used for the transportation of the OPERATING TABLE top to or from the base or pedestal of an OPERATING TABLE with detachable OPERATING TABLE top.

**NOTE** See also 4.2 of the General Standard.

This particular standard does not apply to

- dental PATIENT chairs;
- examination chairs and couches;
- PATIENT-supporting systems of diagnostic and therapeutic devices; (see IEC 60601-2-43)
- OPERATING TABLE heating blankets; (see IEC 80601-2-35)
- PATIENT transfer equipment;
- delivery tables and beds;
- medical beds; (see IEC 60601-2-52)
- field tables.

**NOTE** If OPERATING TABLES will be used in combination with diagnostic and/or therapeutic devices the relevant requirements of each related particular standard ~~have to be considered~~ are also applicable.

##### 201.1.2 Object

*Replacement:*

The object of this particular standard is to establish particular BASIC SAFETY and ESSENTIAL PERFORMANCE requirements for OPERATING TABLES as defined in 201.3.201 ~~and hereinafter also referred to as ME EQUIPMENT~~.

##### 201.1.3 Collateral standards

*Addition:*

This particular standard refers to those applicable collateral standards that are listed in Clause 2 of the general standard and Clause 201.2 of this particular standard.

<sup>1)</sup> The general standard is IEC 60601-1:2005/AMD1:2012, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*.

IEC 60601-1-2 and IEC 60601-1-3 apply as modified in Clauses 202 and 203 respectively. IEC 60601-1-3, IEC 60601-1-8, IEC 60601-1-10, IEC 60601-1-11 and IEC 60601-1-12 do not apply. All other published collateral standards in the IEC 60601-1 series apply as published.

#### 201.1.4 Particular standards

*Replacement:*

In the IEC 60601 series, particular standards may modify, replace or delete requirements contained in the general standard and collateral standards as appropriate for the particular ME EQUIPMENT under consideration, and may add other BASIC SAFETY and ESSENTIAL PERFORMANCE requirements.

A requirement of a particular standard takes priority over the general standard.

For brevity, IEC 60601-1 is referred to in this particular standard as the general standard. Collateral standards are referred to by their document number.

The numbering of clauses and subclauses of this particular standard corresponds to that of the general standard with the prefix "201" (e.g. 201.1 in this standard addresses the content of Clause 1 of the general standard) or applicable collateral standard with the prefix "20x" where x is the final digit(s) of the collateral standard document number (e.g. 202.4 in this particular standard addresses the content of Clause 4 of the IEC 60601-1-2 collateral standard, 203.4 in this particular standard addresses the content of Clause 4 of the IEC 60601-1-3 collateral standard, etc.). The changes to the text of the general standard are specified by the use of the following words:

"Replacement" means that the clause or subclause of the general standard or applicable collateral standard is replaced completely by the text of this particular standard.

"Addition" means that the text of this particular standard is additional to the requirements of the general standard or applicable collateral standard.

"Amendment" means that the clause or subclause of the general standard or applicable collateral standard is amended as indicated by the text of this particular standard.

Subclauses, figures or tables which are additional to those of the general standard are numbered starting from 201.101. However, due to the fact that definitions in the general standard are numbered 3.1 through 3.147, additional definitions in this standard are numbered beginning from 201.3.201. Additional annexes are lettered AA, BB, etc., and additional items aa), bb), etc.

Subclauses, figures or tables which are additional to those of a collateral standard are numbered starting from 20x, where "x" is the number of the collateral standard, e.g. 202 for IEC 60601-1-2, 203 for IEC 60601-1-3, etc.

The term "this standard" is used to make reference to the general standard, any applicable collateral standards and this particular standard taken together.

Where there is no corresponding clause or subclause in this particular standard, the clause or subclause of the general standard or applicable collateral standard, although possibly not relevant, applies without modification; where it is intended that any part of the general standard or applicable collateral standard, although possibly relevant, is not to be applied, a statement to that effect is given in this particular standard.

## 201.2 Normative references

Clause 2 of the general standard applies, except as follows:

*Replacement:*

IEC 60601-1-2:~~2007~~ 2014, *Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral standard: Electromagnetic ~~compatibility~~ disturbances – Requirements and tests*

IEC 60601-1-3:2008, *Medical electrical equipment – Part 1-3: General requirements for basic safety and essential performance – Collateral standard: Radiation protection in diagnostic X-ray equipment*

IEC 60601-1-3:2008/AMD1:2013<sup>2</sup>

*Addition:*

IEC 60601-2-2, *Medical electrical equipment – Part 2-2: Particular requirements for the basic safety and essential performance of high frequency surgical equipment and high frequency surgical accessories*

IEC 60601-2-43, *Medical electrical equipment – Part 2-43: Particular requirements for the basic safety and essential performance of X-ray equipment for interventional procedures*

<sup>2</sup> There exists a consolidated edition 2.1, which includes IEC 60601-1-3:2008 and its Amendment 1 (2013).



IEC 60601-2-46

Edition 3.0 2016-08

# INTERNATIONAL STANDARD

## NORME INTERNATIONALE

Medical electrical equipment –  
Part 2-46: Particular requirements for the basic safety and essential performance  
of operating tables

Appareils électromédicaux –  
Partie 2-46: Exigences particulières pour la sécurité de base et les performances  
essentielles des tables d'opération

## CONTENTS

FOREWORD.....	3
INTRODUCTION.....	5
201.1 Scope, object and related standards .....	6
201.2 Normative references .....	8
201.3 Terms and definitions .....	8
201.4 General requirements.....	9
201.5 General requirements for testing OPERATING TABLES .....	9
201.6 Classification of OPERATING TABLES and ME SYSTEMS.....	9
201.7 OPERATING TABLES identification, marking and documents.....	9
201.8 Protection against electrical HAZARDS from OPERATING TABLES.....	10
201.9 Protection against MECHANICAL HAZARDS of OPERATING TABLES and ME SYSTEMS.....	10
201.10 Protection against unwanted and excessive radiation HAZARDS.....	13
201.11 Protection against excessive temperatures and other HAZARDS.....	13
201.12 Accuracy of controls and instruments and protection against hazardous outputs .....	13
201.13 HAZARDOUS SITUATIONS and fault conditions for OPERATING TABLES .....	14
201.14 PROGRAMMABLE ELECTRICAL MEDICAL SYSTEMS (PEMS) .....	14
201.15 Construction of OPERATING TABLES .....	14
201.16 ME SYSTEMS .....	14
201.17 Electromagnetic compatibility of OPERATING TABLES and ME SYSTEMS.....	14
202 Electromagnetic disturbances – Requirements and tests .....	14
203 Radiation protection in diagnostic X-ray equipment.....	18
Annexes .....	19
Annex G (normative) Protection against HAZARDS of ignition of flammable anaesthetic mixtures .....	20
Annex AA (informative) Particular guidance and rationale .....	21
Bibliography .....	23
Index of defined terms used in this particular standard .....	24
Figure 202.101 – ENCLOSURE ad hoc test .....	16
Figure 202.102 – POWER SUPPLY CORD ad hoc test.....	17
Figure 202.103 – ACCESSORY cable ad hoc test .....	17
Figure AA.1 – Recommended distribution of mass in excess of 135 kg and examples of application .....	21
Table 201.101 – Determination of TENSILE SAFETY FACTOR .....	12
Table AA.1 – Recommended distribution of mass in excess of 135 kg and examples of application .....	22

## INTERNATIONAL ELECTROTECHNICAL COMMISSION

### MEDICAL ELECTRICAL EQUIPMENT –

#### Part 2-46: Particular requirements for the basic safety and essential performance of operating tables

#### FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International standard IEC 60601-2-46 has been prepared by IEC subcommittee 62D Electromedical equipment, of IEC technical committee 62: Electrical equipment in medical practice.

This third edition cancels and replaces the second edition published in 2010 and constitutes a technical revision. This edition of IEC 60601-2-46 was revised to align structurally with the 2005 edition of IEC 60601-1 and with IEC 60601-1:2005/AMD1:2012.

The text of this standard is based on the following documents:

FDIS	Report on voting
62D/1365/FDIS	62D/1371/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

In this standard, the following print types are used:

- Requirements and definitions: roman type.
- *Test specifications: italic type.*
- Informative material appearing outside of tables, such as notes, examples and references: in smaller type. Normative text of tables is also in a smaller type.
- TERMS DEFINED IN CLAUSE 3 OF THE GENERAL STANDARD, IN THIS PARTICULAR STANDARD OR AS NOTED: SMALL CAPITALS.

In referring to the structure of this standard, the term

- “clause” means one of the numbered divisions within the table of contents, inclusive of all subdivisions (e.g. Clause 7 includes subclauses 7.1, 7.2, etc.);
- “subclause” means a numbered subdivision of a clause (e.g. 7.1, 7.2 and 7.2.1 are all subclauses of Clause 7).

References to clauses within this standard are preceded by the term “Clause” followed by the clause number. References to subclauses within this particular standard are by number only.

In this standard, the conjunctive “or” is used as an “inclusive or” so a statement is true if any combination of the conditions is true.

The verbal forms used in this standard conform to usage described in Annex H of the ISO/IEC Directives, Part 2. For the purposes of this standard, the auxiliary verb:

- “shall” means that compliance with a requirement or a test is mandatory for compliance with this standard;
- “should” means that compliance with a requirement or a test is recommended but is not mandatory for compliance with this standard;
- “may” is used to describe a permissible way to achieve compliance with a requirement or test.

An asterisk (\*) as the first character of a title or at the beginning of a paragraph or table title indicates that there is guidance or rationale related to that item in Annex AA.

A list of all parts of the IEC 60601 series, published under the general title *Medical electrical equipment*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC website under "http://webstore.iec.ch" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

## INTRODUCTION

This particular standard concerns the BASIC SAFETY and ESSENTIAL PERFORMANCE of OPERATING TABLES. It amends and supplements IEC 60601-1 (third edition, 2005) and its Amendment 1 (IEC 60601-1:2005/AMD1:2012), hereinafter referred to as the general standard.

The aim of this third edition is to bring this particular standard up to date with reference to the third edition of the general standard through reformatting and technical changes.

The requirements of this particular standard take priority over those of the general standard.

A "General guidance and rationale" for the more important requirements of this particular standard is included in Annex AA. It is considered that knowledge of the reasons for these requirements will not only facilitate the proper application of the standard but will, in due course, expedite any revision necessitated by changes in clinical practice or as a result of developments in technology. However, Annex AA does not form part of the requirements of this Standard.

~~Withdrawing~~

## MEDICAL ELECTRICAL EQUIPMENT –

### Part 2-46: Particular requirements for the basic safety and essential performance of operating tables

#### 201.1 Scope, object and related standards

Clause 1 of the general standard<sup>1)</sup> applies, except as follows:

##### 201.1.1 Scope

*Replacement:*

This particular standard specifies safety requirements for OPERATING TABLES, whether or not having electrical parts, including TRANSPORTERS, used for the transportation of the OPERATING TABLE top to or from the base or pedestal of an OPERATING TABLE with detachable OPERATING TABLE top.

**NOTE** See also 4.2 of the General Standard.

This particular standard does not apply to

- dental PATIENT chairs;
- examination chairs and couches;
- PATIENT-supporting systems of diagnostic and therapeutic devices; (see IEC 60601-2-43)
- OPERATING TABLE heating blankets; (see IEC 80601-2-35)
- PATIENT transfer equipment;
- delivery tables and beds;
- medical beds; (see IEC 60601-2-52)
- field tables.

If OPERATING TABLES will be used in combination with diagnostic and/or therapeutic devices the relevant requirements of each related particular standard are also applicable.

##### 201.1.2 Object

*Replacement:*

The object of this particular standard is to establish particular BASIC SAFETY and ESSENTIAL PERFORMANCE requirements for OPERATING TABLES as defined in 201.3.201.

##### 201.1.3 Collateral standards

*Addition:*

This particular standard refers to those applicable collateral standards that are listed in Clause 2 of the general standard and Clause 201.2 of this particular standard.

<sup>1)</sup> The general standard is IEC 60601-1:2005/AMD1:2012, *Medical electrical equipment – Part 1: General requirements for basic safety and essential performance*.

IEC 60601-1-2 and IEC 60601-1-3 apply as modified in Clauses 202 and 203 respectively. IEC 60601-1-8, IEC 60601-1-10, IEC 60601-1-11 and IEC 60601-1-12 do not apply. All other published collateral standards in the IEC 60601-1 series apply as published.

#### 201.1.4 Particular standards

*Replacement:*

In the IEC 60601 series, particular standards may modify, replace or delete requirements contained in the general standard and collateral standards as appropriate for the particular ME EQUIPMENT under consideration, and may add other BASIC SAFETY and ESSENTIAL PERFORMANCE requirements.

A requirement of a particular standard takes priority over the general standard.

For brevity, IEC 60601-1 is referred to in this particular standard as the general standard. Collateral standards are referred to by their document number.

The numbering of clauses and subclauses of this particular standard corresponds to that of the general standard with the prefix "201" (e.g. 201.1 in this standard addresses the content of Clause 1 of the general standard) or applicable collateral standard with the prefix "20x" where x is the final digit(s) of the collateral standard document number (e.g. 202.4 in this particular standard addresses the content of Clause 4 of the IEC 60601-1-2 collateral standard, 203.4 in this particular standard addresses the content of Clause 4 of the IEC 60601-1-3 collateral standard, etc.). The changes to the text of the general standard are specified by the use of the following words:

"Replacement" means that the clause or subclause of the general standard or applicable collateral standard is replaced completely by the text of this particular standard.

"Addition" means that the text of this particular standard is additional to the requirements of the general standard or applicable collateral standard.

"Amendment" means that the clause or subclause of the general standard or applicable collateral standard is amended as indicated by the text of this particular standard.

Subclauses, figures or tables which are additional to those of the general standard are numbered starting from 201.101. However, due to the fact that definitions in the general standard are numbered 3.1 through 3.147, additional definitions in this standard are numbered beginning from 201.3.201. Additional annexes are lettered AA, BB, etc., and additional items aa), bb), etc.

Subclauses, figures or tables which are additional to those of a collateral standard are numbered starting from 20x, where "x" is the number of the collateral standard, e.g. 202 for IEC 60601-1-2, 203 for IEC 60601-1-3, etc.

The term "this standard" is used to make reference to the general standard, any applicable collateral standards and this particular standard taken together.

Where there is no corresponding clause or subclause in this particular standard, the clause or subclause of the general standard or applicable collateral standard, although possibly not relevant, applies without modification; where it is intended that any part of the general standard or applicable collateral standard, although possibly relevant, is not to be applied, a statement to that effect is given in this particular standard.

## 201.2 Normative references

Clause 2 of the general standard applies, except as follows:

*Replacement:*

IEC 60601-1-2:2014, *Medical electrical equipment – Part 1-2: General requirements for basic safety and essential performance – Collateral standard: Electromagnetic disturbances – Requirements and tests*

IEC 60601-1-3:2008, *Medical electrical equipment – Part 1-3: General requirements for basic safety and essential performance – Collateral standard: Radiation protection in diagnostic X-ray equipment*

IEC 60601-1-3:2008/AMD1:2013<sup>2</sup>

*Addition:*

IEC 60601-2-2, *Medical electrical equipment – Part 2-2: Particular requirements for the basic safety and essential performance of high frequency surgical equipment and high frequency surgical accessories*

IEC 60601-2-43, *Medical electrical equipment – Part 2-43: Particular requirements for the basic safety and essential performance of X-ray equipment for interventional procedures*

---

<sup>2</sup> There exists a consolidated edition 2.1, which includes IEC 60601-1-3:2008 and its Amendment 1 (2013).

## SOMMAIRE

AVANT-PROPOS .....	27
INTRODUCTION .....	30
201.1 Domaine d'application, objet et normes connexes .....	31
201.2 Références normatives .....	33
201.3 Termes et définitions .....	33
201.4 Exigences générales .....	34
201.5 Exigences générales relatives aux essais des TABLES D'OPERATION .....	34
201.6 Classification des TABLES D'OPERATION et DES SYSTEMES EM .....	35
201.7 Identification, marquage et documentation des TABLES D'OPERATION .....	35
201.8 Protection contre les DANGERS d'origine électrique provenant des TABLES D'OPERATION .....	35
201.9 Protection contre les DANGERS MECANIQUES des TABLES D'OPERATION et SYSTEMES EM .....	35
201.10 Protection contre les DANGERS dus aux rayonnements involontaires ou excessifs .....	39
201.11 Protection contre les températures excessives et les autres DANGERS .....	39
201.12 Précision des commandes, des instruments et protection contre les caractéristiques de sortie présentant des risques .....	39
201.13 SITUATIONS DANGEREUSES et conditions de défaut pour les TABLES D'OPERATION .....	39
201.14 SYSTEMES ELECTROMEDICAUX PROGRAMMABLES (SEMP) .....	40
201.15 Construction des TABLES D'OPERATION .....	40
201.16 SYSTEMES EM .....	40
201.17 Compatibilité électromagnétique des TABLES D'OPERATION et des SYSTEMES EM .....	40
202 Perturbations électromagnétiques – Exigences et essais .....	40
203 Radioprotection dans les appareils à rayonnement X de diagnostic .....	44
Annexes .....	45
Annexe G (normative) Protection contre les DANGERS d'inflammation des mélanges anesthésiques inflammables .....	46
Annexe AA (informative) Lignes directrices particulières et justifications .....	47
Bibliographie .....	49
Index des termes définis utilisés dans la présente norme particulière .....	50
Figure 202.101 – Essais ad hoc de l'ENVELOPPE .....	42
Figure 202.102 – Essai ad hoc du CÂBLE D'ALIMENTATION .....	43
Figure 202.103 – Essai ad hoc de l'ACCESSOIRE .....	43
Figure AA.1 – Répartition recommandée de la masse supérieure à 135 kg et exemples d'application .....	47
Tableau 201.101 – Détermination du FACTEUR DE SECURITE EN TRACTION .....	38
Tableau AA.1 – Répartition recommandée de la masse supérieure à 135 kg et exemples d'application .....	48

## COMMISSION ÉLECTROTECHNIQUE INTERNATIONALE

### APPAREILS ÉLECTROMÉDICAUX –

#### Partie 2-46: Exigences particulières pour la sécurité de base et les performances essentielles des tables d'opération

#### AVANT-PROPOS

- 1) La Commission Electrotechnique Internationale (IEC) est une organisation mondiale de normalisation composée de l'ensemble des comités électrotechniques nationaux (Comités nationaux de l'IEC). L'IEC a pour objet de favoriser la coopération internationale pour toutes les questions de normalisation dans les domaines de l'électricité et de l'électronique. A cet effet, l'IEC – entre autres activités – publie des Normes internationales, des Spécifications techniques, des Rapports techniques, des Spécifications accessibles au public (PAS) et des Guides (ci-après dénommés "Publication(s) de l'IEC"). Leur élaboration est confiée à des comités d'études, aux travaux desquels tout Comité national intéressé par le sujet traité peut participer. Les organisations internationales, gouvernementales et non gouvernementales, en liaison avec l'IEC, participent également aux travaux. L'IEC collabore étroitement avec l'Organisation Internationale de Normalisation (ISO), selon des conditions fixées par accord entre les deux organisations.
- 2) Les décisions ou accords officiels de l'IEC concernant les questions techniques représentent, dans la mesure du possible, un accord international sur les sujets étudiés, étant donné que les Comités nationaux de l'IEC intéressés sont représentés dans chaque comité d'études.
- 3) Les Publications de l'IEC se présentent sous la forme de recommandations internationales et sont agréées comme telles par les Comités nationaux de l'IEC. Tous les efforts raisonnables sont entrepris afin que l'IEC s'assure de l'exactitude du contenu technique de ses publications; l'IEC ne peut pas être tenue responsable de l'éventuelle mauvaise utilisation ou interprétation qui en est faite par un quelconque utilisateur final.
- 4) Dans le but d'encourager l'uniformité internationale, les Comités nationaux de l'IEC s'engagent, dans toute la mesure possible, à appliquer de façon transparente les Publications de l'IEC dans leurs publications nationales et régionales. Toutes divergences entre toutes Publications de l'IEC et toutes publications nationales ou régionales correspondantes doivent être indiquées en termes clairs dans ces dernières.
- 5) L'IEC elle-même ne fournit aucune attestation de conformité. Des organismes de certification indépendants fournissent des services d'évaluation de conformité et, dans certains secteurs, accèdent aux marques de conformité de l'IEC. L'IEC n'est responsable d'aucun des services effectués par les organismes de certification indépendants.
- 6) Tous les utilisateurs doivent s'assurer qu'ils sont en possession de la dernière édition de cette publication.
- 7) Aucune responsabilité ne doit être imputée à l'IEC, à ses administrateurs, employés, auxiliaires ou mandataires, y compris ses experts particuliers et les membres de ses comités d'études et des Comités nationaux de l'IEC, pour tout préjudice causé en cas de dommages corporels et matériels, ou de tout autre dommage de quelque nature que ce soit, directe ou indirecte, ou pour supporter les coûts (y compris les frais de justice) et les dépenses découlant de la publication ou de l'utilisation de cette Publication de l'IEC ou de toute autre Publication de l'IEC, ou au crédit qui lui est accordé.
- 8) L'attention est attirée sur les références normatives citées dans cette publication. L'utilisation de publications référencées est obligatoire pour une application correcte de la présente publication.
- 9) L'attention est attirée sur le fait que certains des éléments de la présente Publication de l'IEC peuvent faire l'objet de droits de brevet. L'IEC ne saurait être tenue pour responsable de ne pas avoir identifié de tels droits de brevets et de ne pas avoir signalé leur existence.

La Norme internationale IEC 60601-2-46 a été établie par le sous-comité 62D de l'IEC: Appareils électromédicaux, du comité d'études 62 de l'IEC: Équipements électriques dans la pratique médicale.

Cette troisième édition annule et remplace la deuxième édition parue en 2010. Cette édition constitue une révision technique. La présente édition de l'IEC 60601-2-46 a été révisée de façon à s'aligner sur la structure de l'édition 2005 de l'IEC 60601-1 et de l'IEC 60601-1:2005/AMD1:2012.

Le texte de cette norme est issu des documents suivants:

FDIS	Rapport de vote
62D/1365/FDIS	62D/1371/RVD

Le rapport de vote indiqué dans le tableau ci-dessus donne toute information sur le vote ayant abouti à l'approbation de cette norme.

Cette publication a été rédigée selon les Directives ISO/IEC, Partie 2.

Dans la présente norme, les caractères d'imprimerie suivants sont utilisés:

- Exigences et définitions: caractères romains.
- *Modalités d'essais: caractères italiques.*
- Indications de nature informative apparaissant hors des tableaux, comme les notes, les exemples et les références: petits caractères romains. Le texte normatif à l'intérieur des tableaux est également en petits caractères.
- TERMES DEFINIS A L'ARTICLE 3 DE LA NORME GENERALE, DANS LA PRESENTE NORME PARTICULIERE OU COMME NOTES: PETITES MAJUSCULES.

Concernant la structure de la présente norme, le terme

- "article" désigne l'une des sections numérotées dans la table des matières, avec toutes ses subdivisions (par exemple, l'Article 7 inclut les paragraphes 7.1, 7.2, etc.);
- "paragraphe" désigne une subdivision numérotée d'un article (par exemple, 7.1, 7.2 et 7.2.1 sont tous des paragraphes appartenant à l'Article 7).

Dans la présente norme, les références à des articles sont précédées du mot "Article" suivi du numéro de l'article concerné. Dans la présente norme particulière, les références aux paragraphes utilisent uniquement le numéro du paragraphe concerné.

Dans la présente norme, la conjonction "ou" est utilisée avec la valeur d'un "ou inclusif", ainsi un énoncé est vrai si une combinaison des conditions quelle qu'elle soit est vraie.

Les formes verbales utilisées dans la présente norme sont conformes à l'usage donné à l'Annexe H des Directives ISO/IEC, Partie 2. Pour les besoins de la présente norme:

- "devoir" mis au présent de l'indicatif signifie que la satisfaction à une exigence ou à un essai est obligatoire pour la conformité à la présente norme;
- "il convient/il est recommandé" signifie que la satisfaction à une exigence ou à un essai est recommandée mais n'est pas obligatoire pour la conformité à la présente norme;
- "pouvoir" mis au présent de l'indicatif est utilisé pour décrire un moyen admissible pour satisfaire à une exigence ou à un essai.

Lorsqu'un astérisque (\*) est utilisé comme premier caractère devant un titre, ou au début d'un titre d'alinéa ou de tableau, il indique l'existence d'une ligne directrice ou d'une justification à consulter à l'Annexe AA.

Une liste de toutes les parties de la série IEC 60601, publiées sous le titre général *Appareils électromédicaux*, peut être consultée sur le site web de l'IEC.

Le comité a décidé que le contenu de cette publication ne sera pas modifié avant la date de stabilité indiquée sur le site web de l'IEC sous "http://webstore.iec.ch" dans les données relatives à la publication recherchée. A cette date, la publication sera

- reconduite,
- supprimée,
- remplacée par une édition révisée, ou
- amendée.

Withdrawn

## INTRODUCTION

La présente norme particulière concerne la SECURITE DE BASE et les PERFORMANCES ESSENTIELLES des TABLES D'OPERATION. Elle modifie et complète l'IEC 60601-1 (troisième édition, 2005) et son Amendement 1 (IEC 60601-1:2005/AMD1:2012), appelée norme générale dans la suite du texte.

L'objectif de cette troisième édition est de mettre à jour la présente norme particulière par rapport à la troisième édition de la norme générale par une remise en forme et l'introduction de modifications techniques.

Les exigences de la présente norme particulière prévalent sur celles de la norme générale.

Des lignes directrices et les justifications relatives aux exigences les plus importantes de la présente norme particulière sont fournies dans l'Annexe AA. On considère que la connaissance des raisons qui ont conduit à énoncer ces exigences non seulement facilitera l'application correcte de la norme, mais accélérera en son temps toute révision rendue nécessaire par suite de changements dans la pratique clinique ou d'évolutions technologiques. L'Annexe AA ne fait cependant pas partie des exigences de la présente norme.



## APPAREILS ÉLECTROMÉDICAUX –

### Partie 2-46: Exigences particulières pour la sécurité de base et les performances essentielles des tables d'opération

#### 201.1 Domaine d'application, objet et normes connexes

L'Article 1 de la norme générale<sup>1)</sup> s'applique, à l'exception de ce qui suit:

##### 201.1.1 Domaine d'application

*Remplacement:*

La présente norme particulière spécifie les exigences de sécurité applicables aux TABLES D'OPERATION, que celles-ci comportent ou non des parties électriques, y compris les CHARIOTS DE TRANSFERT, utilisés pour le transport du plateau de la TABLE D'OPERATION vers ou depuis la base ou le socle d'une TABLE D'OPERATION à plateau mobile.

NOTE Voir également 4.2 de la norme générale.

La présente norme particulière ne concerne pas

- les fauteuils dentaires pour PATIENTS;
- les fauteuils et lits d'examen;
- les systèmes de support du PATIENT des appareils de diagnostic et de thérapie; (voir l'IEC 60601-2-43)
- les couvertures chauffantes des TABLES D'OPERATION; (voir l'IEC 80601-2-35)
- les dispositifs de transfert des PATIENTS;
- les tables et lits d'accouchement;
- les lits médicaux; (voir l'IEC 60601-2-52)
- les tables d'opération de campagne.

Si les TABLES D'OPERATION sont destinées à être utilisées en combinaison avec des appareils de diagnostic et/ou de thérapie, les exigences applicables de chaque norme particulière correspondante sont également applicables.

##### 201.1.2 Objet

*Remplacement:*

L'objet de la présente norme particulière est d'établir des exigences particulières pour la SECURITE DE BASE et les PERFORMANCES ESSENTIELLES applicables aux TABLES D'OPERATION, telles que définies en 201.3.201.

<sup>1)</sup> La norme générale est l'IEC 60601-1:2005/AMD1:2012, *Appareils électromédicaux – Partie 1: Exigences générales pour la sécurité de base et les performances essentielles*.

### 201.1.3 Normes collatérales

*Addition:*

La présente norme particulière fait référence aux normes collatérales applicables énumérées à l'Article 2 de la norme générale et à l'Article 201.2 de la présente norme particulière.

L'IEC 60601-1-2 et l'IEC 60601-1-3 s'appliquent telles que modifiées respectivement par les Articles 202 et 203. L'IEC 60601-1-8, l'IEC 60601-1-10, l'IEC 60601-1-11 et l'IEC 60601-1-12 ne s'appliquent pas. Toutes les autres normes collatérales publiées dans la série IEC 60601-1 s'appliquent, telles qu'elles sont publiées.

### 201.1.4 Normes particulières

*Remplacement:*

Dans la série IEC 60601, des normes particulières peuvent modifier, remplacer ou supprimer des exigences contenues dans la norme générale et dans les normes collatérales en fonction de ce qui est approprié à l'APPAREIL EM considéré, et elles peuvent ajouter d'autres exigences de SECURITE DE BASE et de PERFORMANCES ESSENTIELLES.

Une exigence d'une norme particulière prévaut sur l'exigence correspondante de la norme générale.

Par souci de concision, l'IEC 60601-1 est désignée dans la présente norme particulière, par le terme "norme générale". Les normes collatérales sont désignées par leur numéro de document.

La numérotation des articles et paragraphes de la présente norme particulière correspond à celle de la norme générale avec le préfixe "201" (par exemple, 201.1 dans la présente norme aborde le contenu de l'Article 1 de la norme générale) ou de la norme collatérale applicable avec le préfixe "20x", où x est (sont) le (les) dernier(s) chiffre(s) du numéro de document de la norme collatérale (par exemple, 202.4 dans la présente norme particulière aborde le contenu de l'Article 4 de la norme collatérale IEC 60601-1-2, 203.4 dans la présente norme particulière aborde le contenu de l'Article 4 de la norme collatérale IEC 60601-1-3, etc.). Les modifications apportées au texte de la norme générale sont spécifiées par l'utilisation des termes suivants:

"Remplacement" signifie que l'article ou le paragraphe de la norme générale ou de la norme collatérale applicable est remplacé complètement par le texte de la présente norme particulière.

"Addition" signifie que le texte de la présente norme particulière vient s'ajouter aux exigences de la norme générale ou de la norme collatérale applicable.

"Amendement" signifie que l'article ou le paragraphe de la norme générale ou de la norme collatérale applicable est modifié comme indiqué par le texte de la présente norme particulière.

Les paragraphes, figures ou tableaux qui sont ajoutés à ceux de la norme générale sont numérotés à partir de 201.101. Toutefois, en raison du fait que les définitions dans la norme générale sont numérotées 3.1 à 3.147, les définitions complémentaires dans la présente norme sont numérotées à partir de 201.3.201. Les annexes complémentaires sont notées AA, BB, etc., et les alinéas complémentaires aa), bb), etc.

Les paragraphes, figures ou tableaux qui sont ajoutés à ceux d'une norme collatérale sont numérotés à partir de 20x, où "x" est le chiffre de la norme collatérale, par exemple 202 pour l'IEC 60601-1-2, 203 pour l'IEC 60601-1-3, etc.

L'expression "la présente norme" est utilisée pour faire référence à la norme générale, à toutes les normes collatérales applicables et à la présente norme particulière, considérées ensemble.

Lorsque la présente norme particulière ne comprend pas d'article ou de paragraphe correspondant, l'article ou le paragraphe de la norme générale ou de la norme collatérale applicable, bien qu'il puisse être sans objet, s'applique sans modification; lorsqu'il est demandé qu'une partie quelconque de la norme générale ou de la norme collatérale applicable, bien que potentiellement pertinente, ne s'applique pas, cela est expressément mentionné dans la présente norme particulière.

## 201.2 Références normatives

L'Article 2 de la norme générale s'applique, à l'exception de ce qui suit:

*Remplacement:*

IEC 60601-1-2:2014, *Appareils électromédicaux – Partie 1-2: Exigences générales pour la sécurité de base et les performances essentielles – Norme collatérale: Perturbations électromagnétiques – Exigences et essais*

IEC 60601-1-3:2008, *Appareils électromédicaux – Partie 1-3: Exigences générales pour la sécurité de base et les performances essentielles – Norme collatérale: Radioprotection dans les appareils à rayonnement X de diagnostic*  
IEC 60601-1-3:2008/AMD1:2013<sup>2</sup>

*Addition:*

IEC 60601-2-2, *Appareils électromédicaux – Partie 2-2: Exigences particulières pour la sécurité de base et les performances essentielles des appareils d'électrochirurgie à courant haute fréquence et des accessoires d'électrochirurgie à courant haute fréquence*

IEC 60601-2-43, *Appareils électromédicaux – Partie 2-43: Exigences particulières pour la sécurité de base et les performances essentielles des appareils à rayonnement X lors d'interventions*

<sup>2</sup> Il existe une édition consolidée 2.1 qui comprend l'IEC 60601-1-3:2008 et son Amendement 1 (2013).