

TECHNICAL SPECIFICATION

IEC TS 62462

First edition
2007-05

**Ultrasonics – Output test –
Guide for the maintenance of
ultrasound physiotherapy systems**

Withdrawn



Commission Electrotechnique Internationale
International Electrotechnical Commission
Международная Электротехническая Комиссия

PRICE CODE

U

For price, see current catalogue

CONTENTS

FOREWORD.....	3
INTRODUCTION.....	5
1 Scope.....	6
2 Normative references	6
3 Terms and definitions	6
4 Testing regimes.....	7
4.1 Acceptance testing.....	7
4.2 Weekly testing.....	7
4.3 Annual testing	7
5 Performance testing	8
5.1 Acceptance testing.....	8
5.2 Weekly testing.....	9
5.3 Annual testing	10
5.4 Service requirement	12
Annex A (informative) Rationale for testing.....	14
Annex B (informative) Guidance for testers.....	15
Annex C (informative) Quantitative relative ultrasonic output test using temperature rise	19
Annex D (informative) Quantitative relative ultrasonic output test using calorimetry	21
Annex E (informative) Example of weekly test report	23
Annex F (informative) Example of annual test report.....	24
Annex G (informative) Ultrasound portable power standard.....	28
Bibliography.....	29
Figure 1 – Several examples of how to prepare a set-up to check the distortion on the water surface due to ultrasound.....	12
Figure 2 – Set-up where the slight angle of the treatment head to the vertical may improve the image	13
Figure C.1 – Example of a measurement set-up to measure the temperature rise due to ultrasound in absorbing material.....	20
Figure D.1 – Schematic of equipment used within the calorimeter method for monitoring power output of therapy treatment heads.....	21
Figure F.1 – Example of a power calibration graph for a large applicator head.....	26
Figure F.1 – Example of a power calibration graph for a large applicator head.....	26
Figure F.2 – Example of a power calibration graph for a small applicator head	27

INTERNATIONAL ELECTROTECHNICAL COMMISSION

ULTRASONICS – OUTPUT TEST – GUIDE FOR THE MAINTENANCE OF ULTRASOUND PHYSIOTHERAPY SYSTEMS

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with an IEC Publication.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

The main task of IEC technical committees is to prepare International Standards. In exceptional circumstances, a technical committee may propose the publication of a technical specification when

- the required support cannot be obtained for the publication of an International Standard, despite repeated efforts, or
- the subject is still under technical development or where, for any other reason, there is the future but no immediate possibility of an agreement on an International Standard.

Technical specifications are subject to review within three years of publication to decide whether they can be transformed into International Standards.

IEC 62462, which is a technical specification, has been prepared by IEC technical committee 87: Ultrasonics.

The text of this technical specification is based on the following documents:

Enquiry draft	Report on voting
87/350/DTS	87/362/RVC

Full information on the voting for the approval of this technical specification can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.


NOTE The following print types are used:

- requirements: roman type;
- notes: in small roman type;
- words in **bold** in the text are defined in Clause 3.
- numbers in square brackets refer to the Bibliography.

The committee has decided that the contents of this publication will remain unchanged until the maintenance result date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- transformed into an International standard,
- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

A bilingual version of this publication may be issued at a later date.

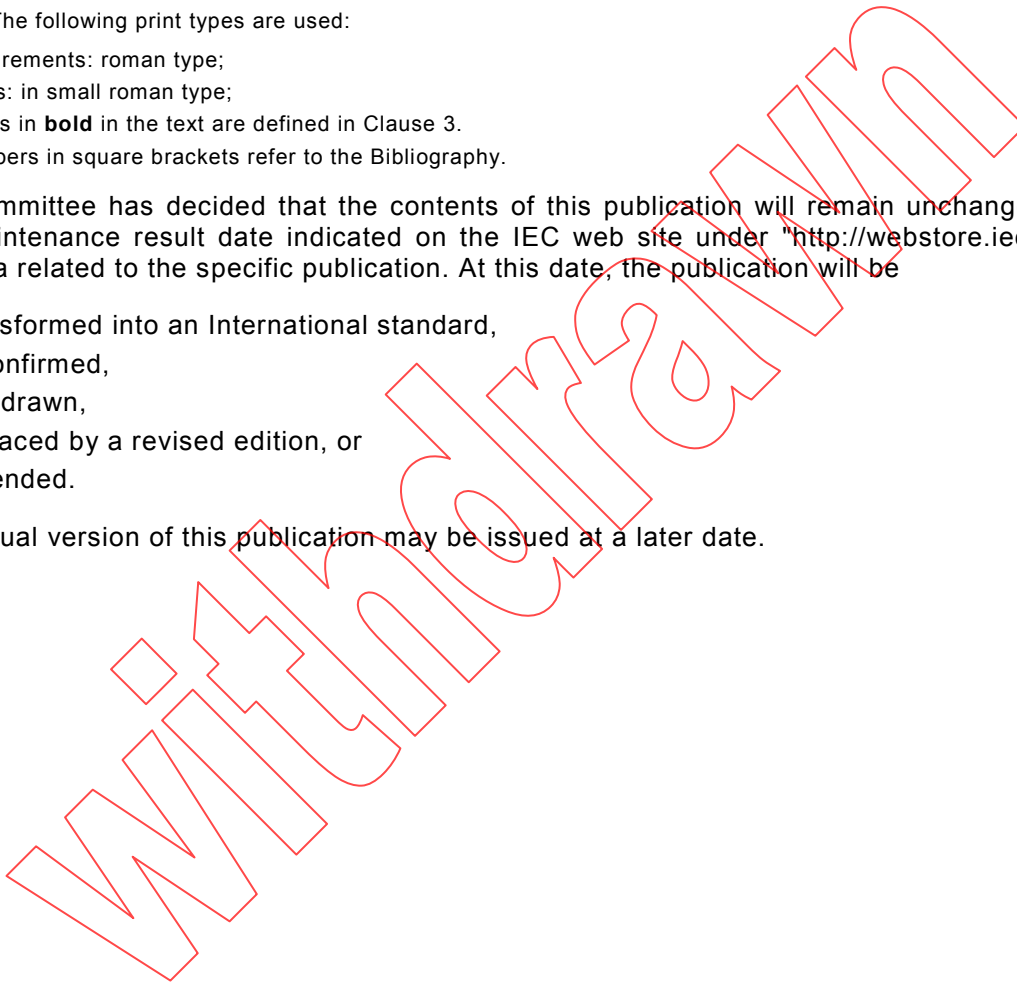

INTRODUCTION

The purpose of this technical specification is to establish standard methods for a qualitative check of the performance of ultrasound physiotherapy devices during their lifetime, and to provide guidance on calibration requirements and techniques.

To ensure that the ultrasound physiotherapy equipment is in an appropriate condition for use, a regular quality check is necessary. This technical specification defines acceptance, weekly and annual checks. The acceptance test checks the delivery of the device and its performance at the start of its lifetime. The weekly check is a simple qualitative check of device operation. In the annual check, in addition to a qualitative check, a quantitative check is defined. Examples are provided of weekly and annual test reports.

This report also gives guidance to the testers concerning the measurement of acoustic output.

Annual testing is to be performed by a skilled tester, e.g. biomedical engineer, medical physicist, medical device service agent, commercial tester, test house, national measurement institute or manufacturer.

Withdrawn

ULTRASONICS – OUTPUT TEST – GUIDE FOR THE MAINTENANCE OF ULTRASOUND PHYSIOTHERAPY SYSTEMS

1 Scope

This technical specification describes methods meant to assist users of ultrasound therapy machines in checking the performance of such machines. It is applicable primarily to physiotherapists, general medical practitioners, chiropractors, osteopaths, beauty therapists, sports professionals, biomedical engineers, medical physicists, medical device service agents, commercial testers, test houses or manufacturers.

NOTE The titles of all publications referred to informatively in this technical specification are listed in the Bibliography.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 61689:2007, *Ultrasonics – Physiotherapy systems – Performance requirements and methods of measurement in the frequency range 0,5 MHz to 5 MHz*

IEC 61161:2006, *Ultrasonics – Power measurement – Radiation force balances and performance requirements*

IEC 60601-2-5, *Medical electrical equipment – Part 2-5: Particular requirements for the safety of ultrasonic physiotherapy equipment*

BIPM, IEC, IFCC, ISO, IUPAC, IUPAP and OIML, *Guide to the expression of uncertainty in measurement*